


Inconclusive — ❤️ -- BPM Average

This ECG is inconclusive due to a poor recording.

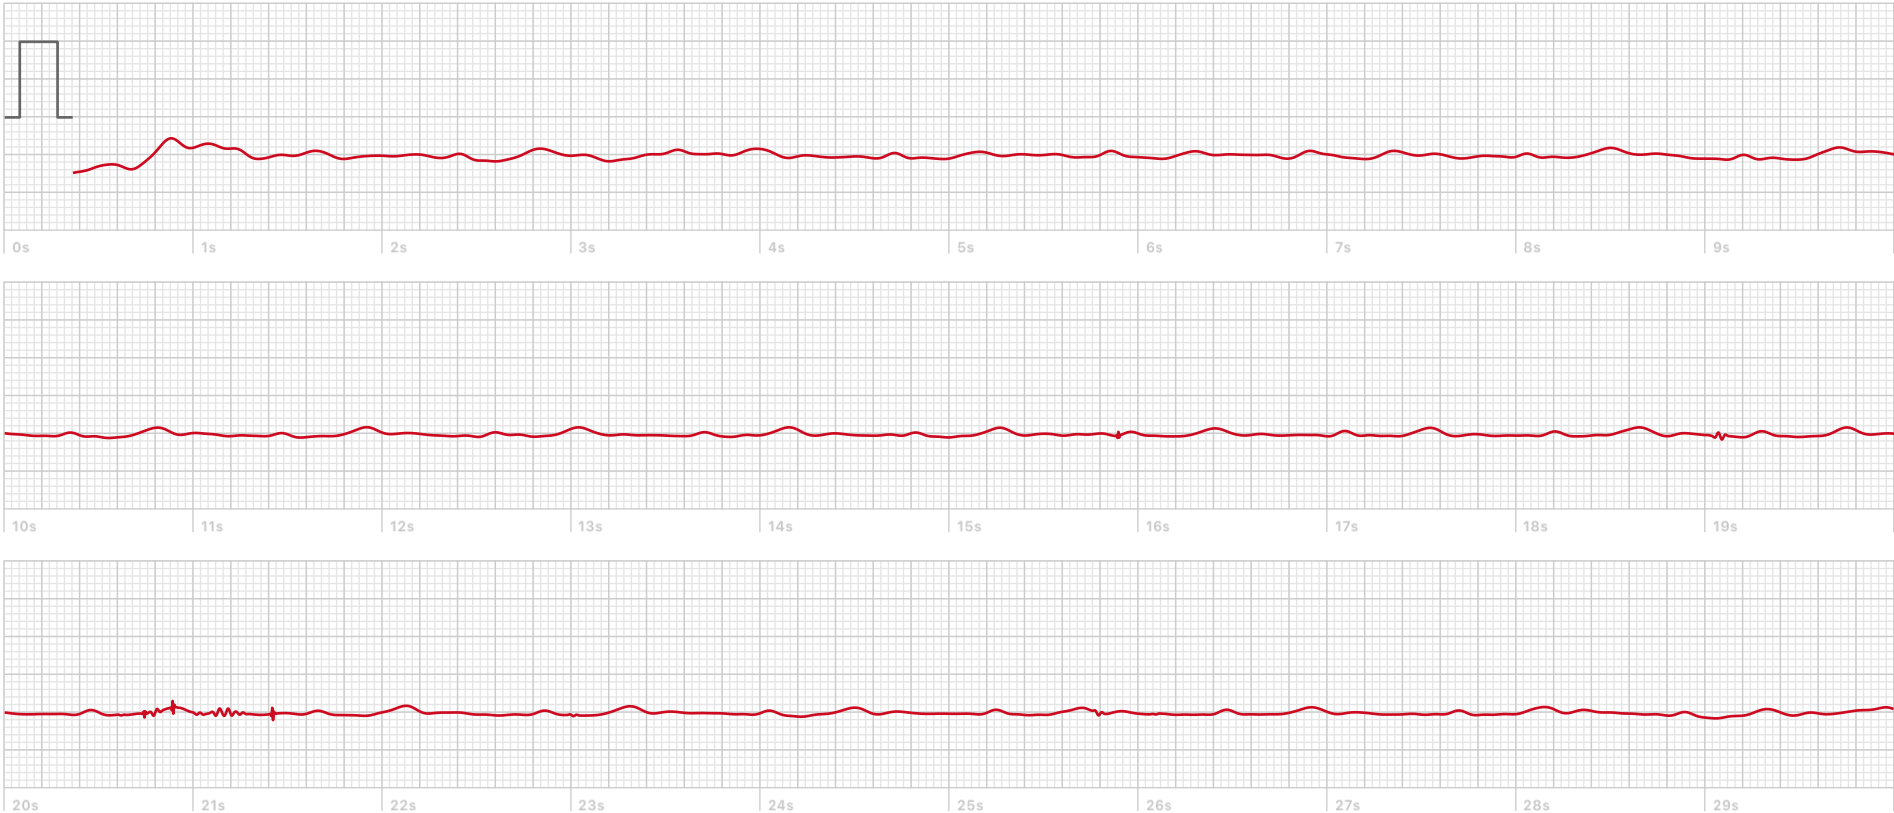

25 mm/s, 10 mm/mV, Lead I, 512Hz, iOS 13.3.1, watchOS 6.1, Watch4,3 — The waveform is similar to a Lead I ECG. For more information, see Instructions for Use.